

AN OCEANOGRAPHIC INSTRUMENTATION SYSTEM

for in situ application *

S. Ben-Yaakov and I. R. Kaplan
 Department of Geology and Institute of
 Geophysics and Planetary Physics
 University of California, Los Angeles 90024

ABSTRACT

An oceanographic instrumentation system has been developed and applied to *in situ* chemical measurements. The system is composed of a submerged assembly and a surface data reduction unit built around a small, general-purpose digital computer (PDP-8/L). The information is recorded digitally by an *in situ* recorder unit, which uses a modified entertainment-type tape recorder to provide eight hours of continuous recording. The resulting data tapes are fed to the computerized data reduction unit that converts the raw data into tabulated physical units. The instrumentation system has been used to measure pH, Eh, temperature and *in situ* carbonate saturation to a depth of 3200 meters.

INTRODUCTION

In a previous paper (Ben-Yaakov and Kaplan, 1968a) we described an oceanographic probe designed for *in situ* measurement. This report describes extended applications of the probe and additional units that provide *in situ* recording and automatic data processing of the information obtained by this oceanographic instrumentation system.

A schematic representation of the original *in situ* probe is depicted in Figure 1a. The unit is supported by an electrical cable which is used as a single channel transmission line to and from the probe. The unit incorporates signal conditioners for the various sensors and a stepping relay that can interconnect any sensor to a voltage-to-frequency converter. The stepping relay is controlled via the electrical cable by a positive going pulse of approximately 30 msec. The output signal of each sensor is thus converted into a proportional frequency signal which is transmitted through the electrical cable to the surface. At

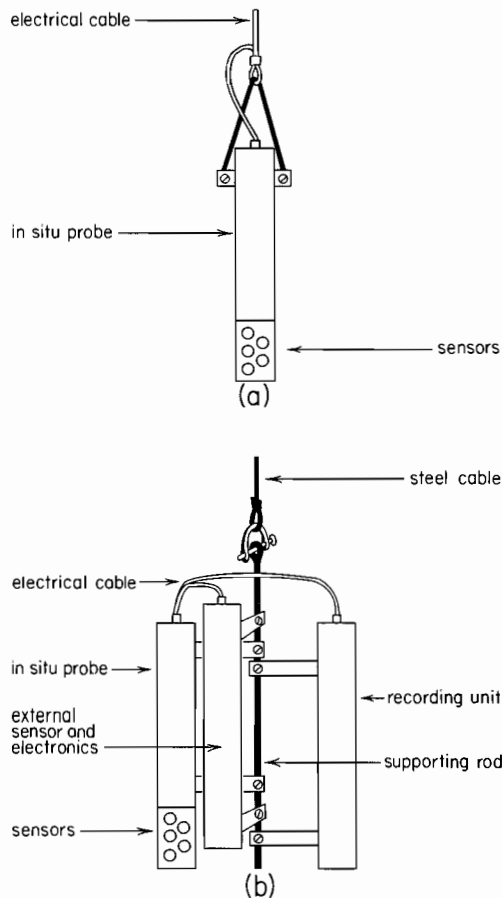


Figure 1. Schematic representation of the original *in situ* unit (a) and the extended *in situ* assembly with a recording unit and an external probe (b).

Reprinted from

MARINE TECHNOLOGY SOCIETY JOURNAL

41

January-February 1971
 Volume 5, No. 1

* Contribution #856, IGPP

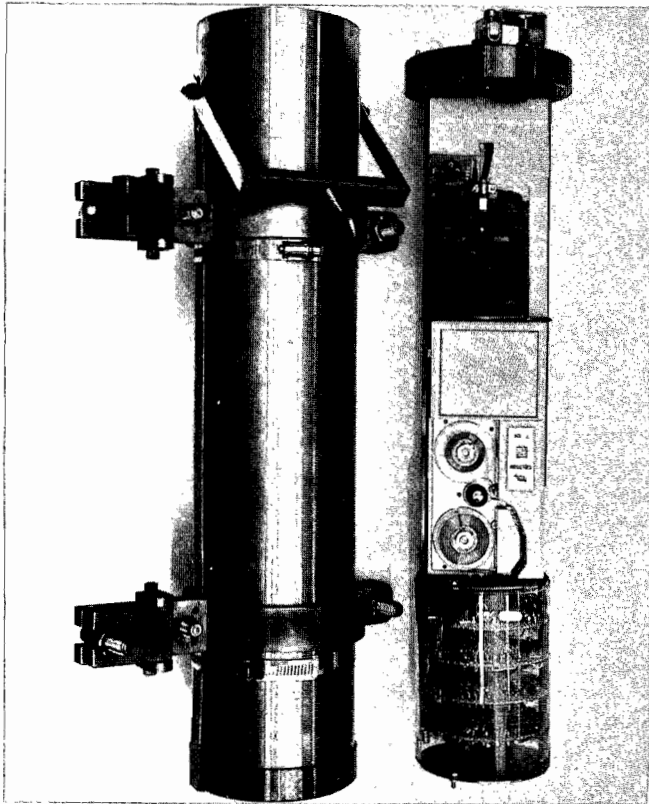


Figure 2. Photograph of the disassembled recording unit.

the surface, the frequency signal can either be measured by a frequency counter or recorded for later manipulation.

The *in situ* unit, as described above, has been used satisfactorily both in the ocean and in lakes to a maximum depth of 1000 meters (Ben-Yaakov and Kaplan, 1968b). In these studies, the frequency was measured by a frequency counter (1 sec. counting time) and recorded manually. The frequency information was converted to physical units by using a desk calculator (Programma 101). This mode of operation has two major drawbacks that limit the practicality of the instrumentation system. These are the needs for an electrical cable and the manual data handling.

An oceanographic electrical cable which is strong enough to support both itself and the *in situ* probe is a very expensive item. Such a cable is highly vulnerable in the

marine environment and will have a short service life. In many applications—and in particular in marine chemistry studies, for which the present system is used—real time measurement is not of prime importance. A delay of a few hours until the data are available can be tolerated. There is therefore, no operational need for the electrical cable, and it should be avoided if possible. A logical solution to overcome the problem of the electrical cable is to use *in situ* recording, so that the probing assembly will be independent and can be supported by regular steel cables which are standard items on any oceanographic vessel. This is the approach adopted in the present study and a recording unit has been developed and constructed.

A schematic representation of the assembly with a cable recording unit is depicted in Figure 1b. In this case we have three units: the probe, a casing for an external sensor and the recording unit. Some of the sensors (such as the conductivity meter) are too large to be incorporated in the casing of the probe itself. It was found more practical to encase such a sensor in a separate housing and to interconnect it to the probe by an electrical cable. The probe, however, will service such a sensor in exactly the same way as any other sensor incorporated within the housing. The present units were designed to withstand a pressure of 10,000 psi which is equivalent to an ocean depth of approximately 6500 meters.

RECORDING UNIT

The recording unit is built around a miniature magnetic tape recorder (Telmar 100T, made in Japan and distributed by Martel, Los Angeles, California) that has external dimensions of 19.5 x 8.5 x 5 cm and a capstan-drive mechanism which is governed by a feedback speed control. The tape recorder was slightly modified in three respects: the amplification circuitry was bypassed feeding the signal directly to the head, a tape spool security lock was incorporated to hold the spools firmly, and the tape speed was decreased. The latter was achieved by adding an extra resistor to the speed control circuit so as to reduce the speed from 15/16 inch per second to approximately 0.125 inches per second. The tape recorder uses tape spools of 1-3/4-inch diameter which will run continuously for four hours, with a 0.5 mil tape and eight hours with 0.25 mil tape. At this low speed, the magnetic head is capable of recording directly (no bias) the frequency band 200-300 Hz. All data are, therefore, modulated with a 250 Hz signal before being fed to the magnetic head.

The recording unit is built into a 4-inch I.D. 21-inch long stainless steel high pressure housing (EG & G type 270) which is rated to 10,000 psi. The unit is built in three sections: the lower electronics compartment, the tape

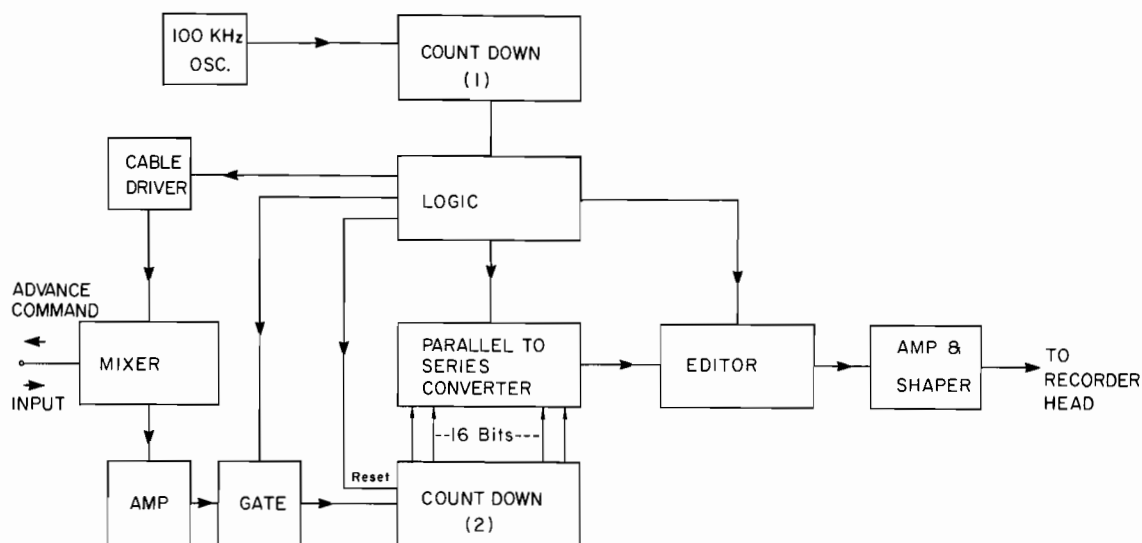


Figure 3. Functional block diagram of the recording unit.

recorder, and the battery pack. The electronics section is protected by a plastic shield to prevent damage when handling the unit. Two high-pressure electrical connectors, at the upper cap of the unit, provide the required electrical connection. Figure 2 is a photograph of the disassembled unit and the block diagram of Figure 3 demonstrates the basic design.

The circuit is basically a frequency counter which counts the incoming signal over a period of 1 second. Counting is done by an IC BCD counters and the result is represented as a four-digit BCD number, namely 16 bits. These parallel bits are converted to a serial string of pulses, edited and fed to the head of the magnetic tape. The unit also provides an "advance" pulse which is sent through the cable to the probe and used to advance the stepping relay. All the timing pulses are derived from a 100 KHz crystal controlled oscillator. Detailed descriptions of the electronic circuitry and logic design is given elsewhere (Ben-Yaakov, 1970).

DATA REDUCTION SYSTEM

The magnetic tapes are processed by a surface system built around a small, general purpose digital computer (PDP 8/L). The basic blocks of this system are depicted in Figure 4. It is composed of another entertainment-type magnetic tape recorder feeding the computer through a read-out unit and a computer interface. The read-out unit rearranges the serially recorded numbers in parallel and produces a pulse whenever a data point is ready to be read into the computer. The tape is played back at 1-7/8 ips, namely 15 times faster than the recording speed, which results in a

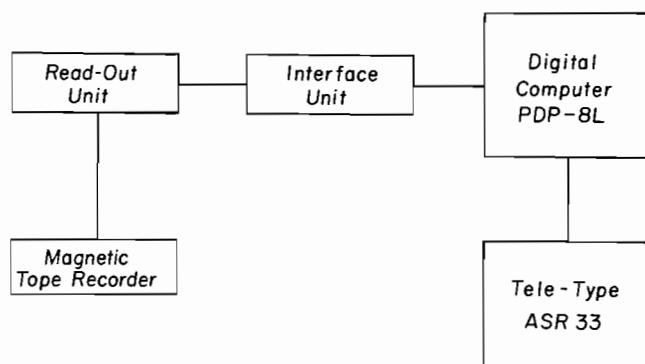


Figure 4. Block diagram of the data reduction system.

data rate of approximately six four-digit numbers per second. The original 250 Hz modulating signal is converted to 3.75 KHz, well within the audio range so that any audio tape recorder can be used to play back the tapes. (We are using the CRAIG 212, which is a small entertainment-type tape recorder).

The use of entertainment-type tape recorders with relatively poor performance, dictated a careful design to ensure reliable readout. The main problems that had to be overcome were inconsistency of the tape speed, wow and flutter. These were overcome by basing the bits and sync identification on the number of cycles (the original 250 Hz modulating signal) which are contained in them. The "zero" bit contains 5 cycles, the "one" bit contains 20

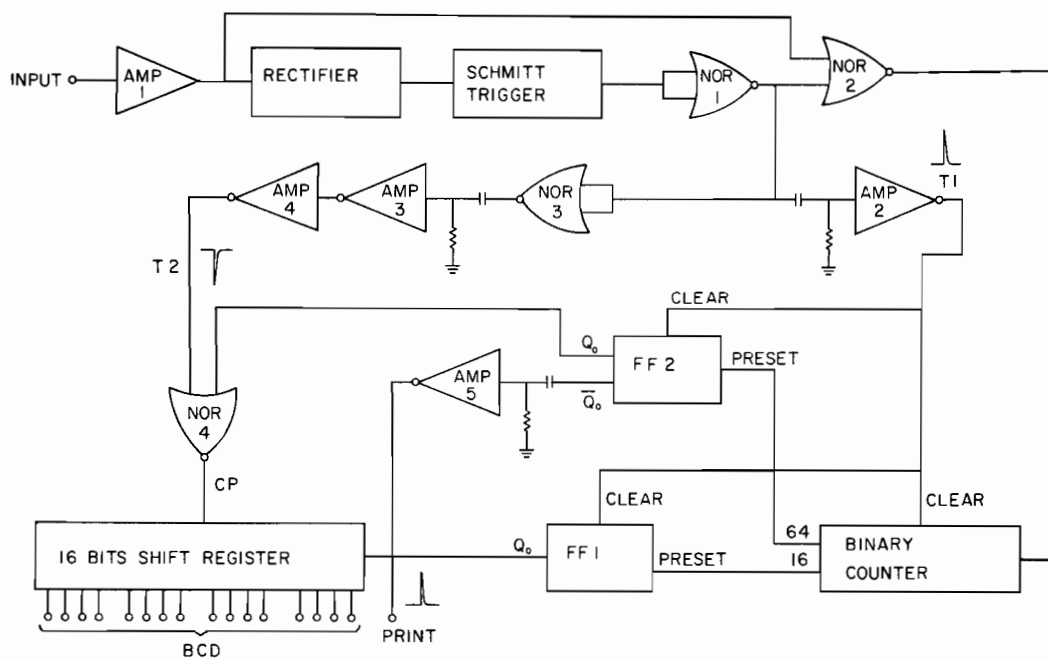


Figure 5. Functional block diagram of the read-out unit.

NUMBER OF DELETIONS: 4
 D(1): 48.0
 D(1): 50.0
 D(1): 95.1
 D(1): 96.5
 PH (MV) MAX: -3.60
 PH (MV) MIN: -3.90
 SCALE: 0.500 MV/DIVISION
 START: 45.0
 END: 110.5

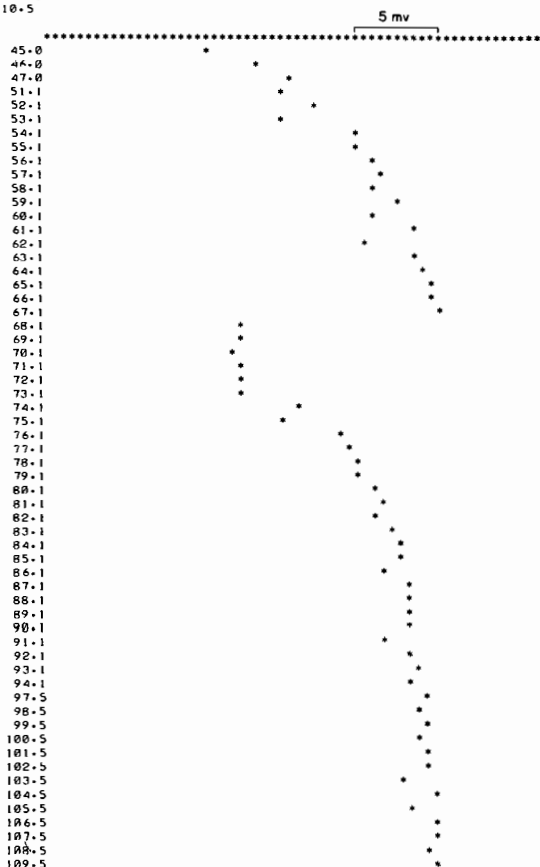


Figure 6. In situ carbonate saturometry. Santa Monica Basin. Station 3. Depth: 100 m.

cycles and the "sync" bit contains at least 75 cycles. Hence, one can identify the various pulses by counting the number of cycles within them. This method is completely independent of the recording or playback speeds as long as the read-out unit is capable of counting the (original) 250 Hz cycles. A block diagram of the read-out unit is depicted in Figure 5.

The interface unit is mainly a gating circuit which facilitates the strobing of the information into the computer accumulator. The output of the read-out unit is compatible with a number of commercially available digital printers (such as Hewlett-Packard 562A or Monsanto 501A), which can be conveniently used on board ship when it is desirable to scan the raw data.

The data are processed in two steps: the information is first translated from the magnetic tape to a perforated paper tape, which is later read by the computer for calculation. The computed results are simultaneously typed on the teletype while punching a paper tape for later manipulation, such as plotting. The two-step process greatly simplifies the programming procedure because a higher level language can be used.

Processing time is mainly controlled by the input-output facilities of the system. Our computer has only the teletype as an input-output device, apart from the magnetic tape recorder that is used initially to read in the raw data. The reading and printing speed of the teletype is 0.1 sec per character, whereas the reading speed of the magnetic tape recorder is approximately 0.05 sec per character. Each data

Table I – A Sample of a Print-Out of Raw Data

```

0585J4548J6908J2423J1347J0403J8560J2032J2030J4163J1271J8012
059J4526J6908J2423J1347J0403J8559J2032J2030J4163J1370J7995
0595J4525J6909J2421J1347J0403J8558J2031J2029J4162J1457J7975
0595J4526J6909J2420J1347J0403J8557J2032J2029J4163J1563J7961
0595J4525J6908J2419J1347J0403J8558J2031J2029J4163J1589J7946
0596J4525J6909J2417J1347J0403J8558J2031J2028J4163J1616J7939
0597J4525J6909J2417J1347J0403J8558J2031J2029J4162J1642J7924
0598J4525J6909J2415J1347J0403J8559J2030J2029J4163J1660J7916
0599J4525J6909J2414J1347J0403J8560J2031J2029J4163J1675J7905
0600J4526J6910J2413J1347J0403J8561J2030J2029J4163J1686J7901
0601J4527J6910J2412J1346J0403J8561J2031J2029J4163J1694J7895
0602J4526J6910J2411J1346J0403J8562J2030J2029J4163J1702J7900
0603J4527J6910J2410J1347J0403J8563J2031J2028J4163J1724J7887
0603J4528J6910J2408J1346J0403J8563J2031J2029J4163J1732J7889
0604J4528J6910J2407J1346J0403J8563J2031J2029J4164J1738J7887
0605J4528J6910J2406J1347J0403J8564J4058J4055J4163J1745
7927J0606J4529J6911J2406J1346J0404J8564J4058J4056J4163J1752
7941J0606J4530J6910J2405J1346J0404J8565J4059J4057J4164J1749
7944J0607J4529J6911J2404J1346J0403J8564J4059J4056J4164J1754
7945J0608J4530J6911J2403J1346J0404J8565J4059J4058J4164J1757
7945J0608J4530J6911J2402J1346J0403J8565J2032J2029J4165J1760
7912J0608J4530J6912J2400J1346J0403J8566J2031J2029J4165J1762
7896J0609J4530J6911J2400J1346J0403J8565J2032J2029J4164J1764
7885J0609J4531J6912J2398J1345J0403J8566J2031J2029J4165J1767
7897J0610J4531J6911J2398J1345J0403J8566J2031J2028J4165J1782
7879J0611J4531J6911J2397J1346J0403J8567J2031J2029J4165J1782
7876J0610J4531J6912J2396J1346J0403J8567J2031J2029J4165J1779
7876J0611J4531J6911J2399J1346J0404J8567J2031J2029J4165J1777
7867J0611J4531J6911J2394J1345J0404J8567J2031J2028J4165J1775
7875J0612J4531J6911J2393J1345J0404J8567J2031J2029J4165J1774
7862J0612J4531J6911J2392J1345J0404J8567J2031J2028J4165J1778
    
```

Table II – A Sample of a Print-Out of Calculated Data

T(M)	D(M)	TEMP	PH(MV)	PH	EH	PUMP	B:
45.0	267.2	8.933	-373.70	8.037	474.62	2029.0	24.100
46.0	265.0	8.933	-372.46	8.015	472.46	2028.0	24.083
47.0	269.6	8.938	-372.60	8.018	471.62	2029.0	24.070
48.0	271.9	8.938	-372.30	8.012	471.12	2029.0	24.060
50.0	271.9	8.949	-377.80	8.110	469.61	4056.0	24.040
51.0	274.2	8.933	-378.06	8.115	470.06	4057.0	24.033
52.0	278.7	8.955	-378.04	8.114	469.47	4056.0	24.027
53.0	276.5	8.944	-378.10	8.116	469.21	4058.0	24.010
54.0	278.7	8.949	-374.64	8.054	468.97	2029.0	24.007
55.0	281.0	8.944	-372.99	8.024	468.74	2029.0	23.984
56.0	281.0	8.960	-372.04	8.007	468.46	2029.0	23.987
57.0	283.3	8.955	-373.09	8.026	468.23	2029.0	23.964
58.0	285.6	8.955	-371.34	7.995	466.77	2028.0	23.967
59.0	283.3	8.949	-371.04	7.989	466.77	2029.0	23.957
60.0	285.6	8.949	-370.99	7.988	467.04	2029.0	23.944
61.0	283.4	8.944	-370.20	7.975	467.31	2029.0	23.970
62.0	285.7	8.944	-371.00	7.989	467.51	2028.0	23.920
63.0	285.7	8.944	-369.70	7.966	467.61	2029.0	23.910
64.0	288.0	8.933	-369.30	7.959	467.22	2028.0	23.900
65.0	285.7	8.944	-369.60	7.964	467.41	2028.0	23.890
66.0	285.6	8.944	-369.04	7.954	467.28	2028.0	23.877
67.0	288.0	8.938	-369.64	7.965	467.28	2028.0	23.877
68.0	288.0	8.949	-368.64	7.947	466.87	2029.0	23.867
69.0	290.2	8.955	-368.59	7.945	465.83	2029.0	23.854
70.0	290.2	8.955	-374.39	8.049	466.23	2047.0	23.854
71.9	290.3	8.949	-377.94	8.113	465.87	4056.0	23.827
72.9	292.5	8.955	-378.08	8.115	464.33	4056.0	23.814
73.9	292.5	8.949	-378.48	8.122	462.04	4057.0	23.814

point is 5 digits (or characters) of information, and since it has to pass four times through the input-output (magnetic to paper tape and paper tape to typed results) it requires approximately 2 seconds read-write time. In practice, the total processing time per character is approximately 2.5 seconds, which is half real time. A complete processing of eight hours real time (one spool) which contains 11,000 numbers is approximately four hours. This processing time, although slow when compared to a large computer installation, is of course a tremendous improvement over manual computation.

The data processing system is small enough in its physical dimension to be brought on board the ship from which the study is being made. This mode of operation is highly desirable, since it provides tabulated results within a few hours, so that the study can be modified according to the data obtained.

The computer data processing system is the most expensive part of our instrumentation system, with a total cost of approximately \$10,000. On the other hand, the *in situ* assembly is relatively inexpensive as a result of a basic philosophy of design which was aimed at reducing the cost of the vulnerable units. This was accomplished by: (1) using time multiplexing, namely measuring one parameter at a time rather than all the parameters simultaneously, (2) making all correction on the raw signal on the surface rather than by analog circuitry *in situ*, and (3) developing a novel, inexpensive recording unit which makes use of an

*C

```

NUMBER OF DELETIONS:0
D(I):0
PH (MV) MAX:-346
PH (MV) MIN:-352
SCALE= 0.100 MV/DIVISION
START:171.6
END:208.7
    
```

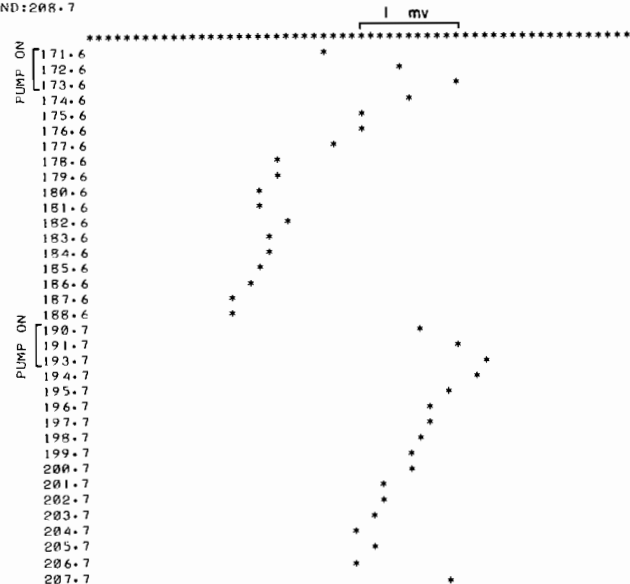


Figure 7. In situ carbonate saturation. Santa Monica Basin. Station 9. Depth: 400 m.

S. BEN-YAAKOV is Acting Assistant Professor of Engineering and Assistant Research Engineer with the Department of Geology, University of California at Los Angeles. He has a BS (Electrical Engineering), from the Israel Institute of Technology, MS and PhD (Engineering) from UCLA. Among his interests are marine sciences instrumentation techniques and applications to chemical oceanography.



ISAAC R. KAPLAN is Professor of Geology and Geophysics at the University of California, at Los Angeles. He received his BSc and MSc (Chemistry) from Canterbury University, New Zealand and PhD (Biogeochemistry) from University of Southern California. His principle interests are marine geochemical studies on the cycling of elements in the ocean and biosphere and diagenesis of organic matter.



entertainment-type tape recorder rather than a professional digital tape recorder. The time multiplexing technique also simplifies addition of new sensors to the probe, since the bulk of the electronic circuitry is shared by all the sensors.

RESULTS

This system presently incorporates five sensors for measuring the following parameters: depth, temperature, pH, Eh, and conductivity of seawater. Two of the sensors, the pressure transducer and the thermistor, have been obtained commercially, whereas the remaining sensors have been developed during the course of this study (Ben-Yaakov 1970). The pH electrode, together with an *in situ* centrifugal pump, has been used to perform an *in situ* carbonate saturometer experiment. In this case, the glass electrode is placed in a cell and surrounded by fine grains of calcite. The cell is connected to the pump by a hose, so that it can be flushed by seawater when the pump is turned on. The pump is powered by a nickel cadmium (NiCd) battery pack and controlled by a timer which fixes the duty cycle. By this arrangement, the pH of the seawater—before and after contact with a solid phase of CaCO_3 —can be measured. This information can then be used to estimate the degree of saturation of the seawater with respect to CaCO_3 .

A print-out sample of the raw data is given in Table I, and a sample of the computer output is shown in Table II. The calculation steps include the correction of the raw data for electronic drift and take into account the calibration data of the various sensors.

The output print-out (Table II) includes the running time (starting from the beginning of the experiment), depth, temperature, mV output of the pH electrode (corrected for electronic drifts), pH, Eh (corrected for

temperature dependence of Ag/AgCl electrode potential), pump marker (4000 when pump is on), and battery voltage. The marker channel is used in the saturometer experiments to indicate when the cell is being flushed. This channel was used for recording salinity measurements in some earlier experiments.

The computer output data have been used to plot the change of the pH electrode output potential during the saturometer cycle. This was accomplished by another program that uses the teletypewriter as a plotter. Figures 6 and 7 are a sample of two plots obtained for two water depths in Santa Monica Basin. These are plots of mV output (horizontal) versus time (vertical). The scale sensitivity (mV/division) may be different for each plot and is indicated on each figure. The mV scale shows positive values to the right. The time scale is in minutes, and each point corresponds to a measurement that was taken during a cycle of the stepping relay. Figure 6, which corresponds to 100 m depth, indicates that the output of the glass electrode became more positive when the seawater was left to equilibrate with the CaCO_3 . This implies that the calcium carbonate was precipitating (Ben-Yaakov and Kaplan, 1969) namely the water was supersaturated with respect to calcite. The data at 400m (figure 7) show a negative voltage shift, which indicates that the water was undersaturated, since CaCO_3 was dissolving. Results and interpretation of the *in situ* carbonate saturometer experiment are given elsewhere (Ben-Yaakov 1970).

ACKNOWLEDGMENTS

We would like to thank Mr. Ed Ruth for assistance in various phases of the laboratory and shipboard studied. We also wish to thank the Los Angeles Sanitation Department, Scripps Institution of Oceanography, Naval Electronics Laboratory, and University of Southern California for making research vessels available to us to undertake equipment tests and field measurements. This study was supported by an AEC contract AT(04-3)-34 PA 178 and a fellowship to S. Ben-Yaakov from the Israel Oceanographic and Limnological Company.

REFERENCES

1. Ben-Yaakov, S. and I. R. Kaplan. 1968a. *A versatile probe for oceanographic in situ measurements*. J. Ocean Tech. 2, (3), p. 25-29.
2. Ben-Yaakov, S. and I. R. Kaplan. 1968b. *pH-Temperature profiles in ocean and lakes using an in situ probe*. Lim. and Oceanogr. 4, p. 688-693.
3. Ben-Yaakov, S. and I. R. Kaplan. 1969. *Determination of carbonate saturation of seawater with a carbonate saturometer*. Lim. and Oceanogr. 14, p. 874-882.
4. Ben-Yaakov, S. 1970. *An oceanographic instrumentation system for in situ measurements*. PhD thesis. University of California, Los Angeles.